

EC Design-Examination Certificate

Directive 93/42/EEC on Medical Devices, Annex II Section 4

No.**CE 73804****Issued To:**

**Johnson & Johnson International
c/o European Logistics Centre
Leonardo Da Vincilaan 15
BE-1831 Diegem
Belgium**

In respect of:

Coated VICRYL™ PLUS Antibacterial (Polyglactin 910) Sterile Synthetic Absorbable Suture

BSI has performed a design examination on the above devices in accordance with the Council Directive 93/42/EEC, Annex II Section 4. The design conforms to the requirements of this directive. For marketing of these products an additional Annex II excluding Section 4 certificate is required.

For and on behalf of BSI, a Notified Body for the above Directive (Notified Body Number 0086):



Stewart Brain, Head of Compliance & Risk -
Medical Devices

First Issued: **2004-09-17**

Date: **2018-06-29**

Expiry Date: **2023-07-04**

...making excellence a habit.™

Page 1 of 6

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.

EC Design-Examination Certificate

Supplementary Information to CE 73804

Issued To:

Johnson & Johnson International
c/o European Logistics Centre
Leonardo Da Vincilaan 15
BE-1831 Diegem
Belgium

Product: Coated VICRYL™ PLUS Antibacterial (Polyglactin 910) Sterile Synthetic Absorbable Suture

SUTURE CHARACTERISTICS	RANGE
Suture Material (Absorbable/Non-Absorbable)	Absorbable
Suture Gauge Size	1.0 – 5.0 (metric)
Suture Length	5cm – 250cm
Suture Dyed/Undyed	Dyed/Undyed
Suture Color (If dyed)	Violet
Coated/Uncoated	Coated (Copolymer of glycolide and lactide, calcium stearate)
Multifilament/Monofilament	Multifilament
Contains Antimicrobials (Yes/No)	Yes
Triclosan Maximum Levels (ug/m)	≤ 275 µg/m
Accessories to suture type	N/A
Needled/Non-Needled	Needled/Non-Needled
Number of Needles per Suture	Single Armed/Double Armed
Needle Material	420, 420 SS, 4310 SS, ETHALLOY
Needle Coating	Silicone, MULTIPASS

First Issued: **2004-09-17**

Date: **2018-06-29**

Expiry Date: **2023-07-04**

...making excellence a habit.™

Page 2 of 6

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.

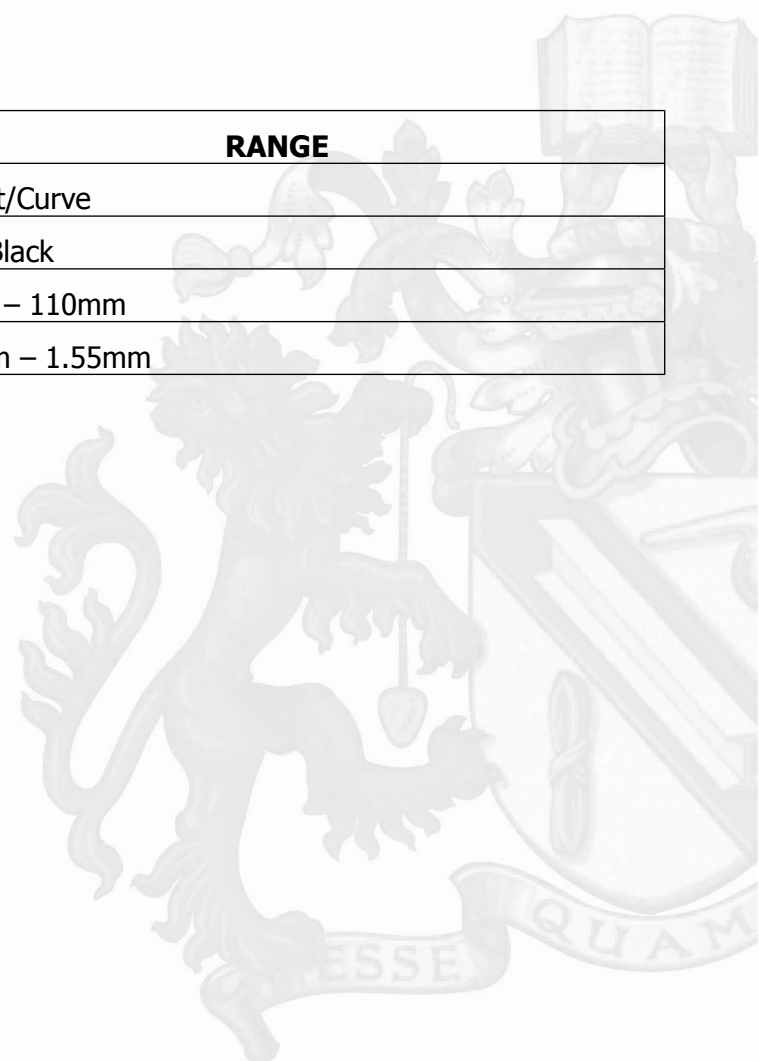
EC Design-Examination Certificate

Supplementary Information to CE 73804

Issued To:

Johnson & Johnson International
c/o European Logistics Centre
Leonardo Da Vincilaan 15
BE-1831 Diegem
Belgium

SUTURE CHARACTERISTICS	RANGE
Needle Shape	Straight/Curve
Needle Color	Silver/Black
Needle Length	3.5mm – 110mm
Needle Wire Diameter	0.10mm – 1.55mm

First Issued: **2004-09-17**Date: **2018-06-29**Expiry Date: **2023-07-04**

...making excellence a habit.™

Page 3 of 6

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.

EC Design-Examination Certificate

Supplementary Information to CE 73804

Issued To:

Johnson & Johnson International
c/o European Logistics Centre
Leonardo Da Vincilaan 15
BE-1831 Diegem
Belgium

Certificate History

Date	Reference Number	Action
17 September 2004	10049224	First issue.
23 December 2004	10063712	Addition of size 4 and 5 sutures.
01 March 2005	10065810	Extension to shelf life of Vicryl Plus suture which contains Triclosan from 2 years to 3.0 years.
20 June 2005	10065925	Transfer of coating process to Hamburg Germany.
12 April 2006	10068862	Changing the upper Triclosan limit to 270 µg/m.
02 June 2006	10078773	Change to pack configuration (addition of Multipack) and minor increase in upper Triclosan limit to 275 µg/m.
09 September 2009	10109409	Certificate renewal.
30 October 2012	10136503	Change of legal manufacturer address. Administrative update to the supplementary page for clarity only. Administrative update to certificate format.

First Issued: **2004-09-17**Date: **2018-06-29**Expiry Date: **2023-07-04**

...making excellence a habit.™

Page 4 of 6

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.

EC Design-Examination Certificate

Supplementary Information to CE 73804

Issued To:

Johnson & Johnson International
c/o European Logistics Centre
Leonardo Da Vincilaan 15
BE-1831 Diegem
Belgium

Date	Reference Number	Action
08 July 2014	10144769	Change of device name to Coated VICRYL™ Plus Antibacterial Suture. Review of updated labelling and instructions for use. Administrative update to certificate format.
11 September 2014	10149209	Certificate renewal. Administrative corrections to product details in supplementary page.
04 December 2015	10153616	Addition of Needle Master File.
18 March 2016	10159048	Change in DuPont™ Tyvek® flash-spinning technology (1073B Transition Tyvek®). Administrative updates to scope and supplementary page.
03 August 2016	10162190	Installation of New Packaging Equipment GIFM1 and Ink Change on the Foil Package. Administrative update to supplemental information.
16 November 2016	10166522	Addition of Ethicon, Inc. Athens, GA for suture raw material manufacturing for sizes USP 4/0, 2/0, 1 (Metric 1.5, 3, 4)(56 Denier, Dyed).
22 December 2016	10153556	Multipack Folder and Coating Solution Change for product codes VCP1219H and VCPV967H.

First Issued: **2004-09-17**

Date: **2018-06-29**

Expiry Date: **2023-07-04**

...making excellence a habit.™

Page 5 of 6

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.

EC Design-Examination Certificate

Supplementary Information to CE 73804

Issued To:

Johnson & Johnson International
c/o European Logistics Centre
Leonardo Da Vincilaan 15
BE-1831 Diegem
Belgium

Date	Reference Number	Action
05 May 2017	10169583	Addition of Ethicon, Inc. Athens, GA for suture raw material manufacturing for sizes USP 9-0 (Metric 0.3) (8 Denier, Dyed), USP 6-0 (Metric 0.7) (14 Denier, Un-Dyed), USP 3-0 (Metric 2) (52 Denier, Dyed & Un-Dyed) and USP 4/0, 2/0, 1 (Metric 1.5, 3, 4) (56 Denier, Un-Dyed).
29 June 2017	8742925	Addition of Ethicon, Inc. Athens, GA for suture raw material manufacturing for sizes USP 8-0 (Metric 0.4) (10 Denier, Dyed), USP 6-0 (Metric 0.7) (14 Denier, Dyed), USP 7-0 (Metric 0.5) (16 Denier, Dyed & Un-Dyed), USP 5-0 (Metric 1) (28 Denier, Dyed), and USP 0 (Metric 3.5) (80 Denier, Dyed & Un-Dyed).
11 August 2017	8716374	Review of BC5 blanking and cartoning machine at San Angelo, TX site.
Current	8942302	Certificate Renewal.

First Issued: **2004-09-17**Date: **2018-06-29**Expiry Date: **2023-07-04**

...making excellence a habit.™

Page 6 of 6

Validity of this certificate is conditional on the quality system being maintained to the requirements of the Directive as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.