



STAIRS WHEEL CHAIR code SED001

Instructions and Maintenance



Fig1



Fig2

HOW TO OPEN THE WHEEL CHAIR

When the chair is folded fig 1, hold both points A and B and push up to the end to reach the Fig. 2

HOW TO PREPARE THE PATIENT TRANSPORTATION

Once the Patient is well seated, lower both the armchair pressurising the end higher part of the plastic protection, as in fig. 3. To bring the back armchair to an horizontal position pull them up.

To pull the front armchair down push and stop when they do click on the lock fig. 4

The lift bars can be lengthen pushing on the button and pulling on the handle towards you. You will get the wheel chair as in fig. 2.



Fig3



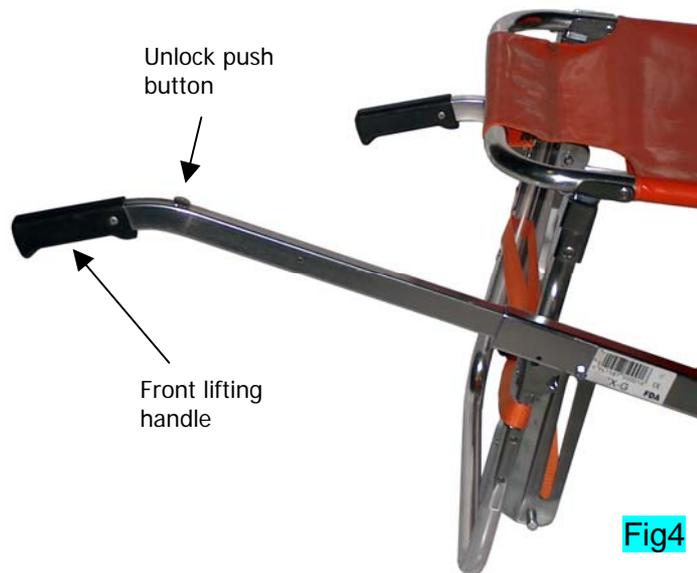


Fig4

SECURITY SYSTEMS

To have a better stability when the chair is open, the left wheel can be locked, fig. 5, pressing the foot on the A point. To unlock press once again with your foot on the B point..

To have the front lift bar at the same position as when the wheel chair is folded, hold the lock as in fig. 6, pull it towards you, freeing the pivot then lift the handle. Quick locked belts are supplied with the wheel chair for the Patient security

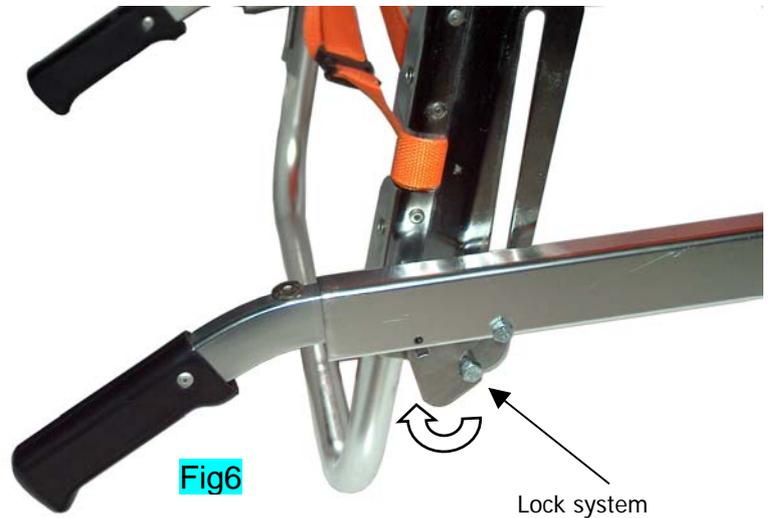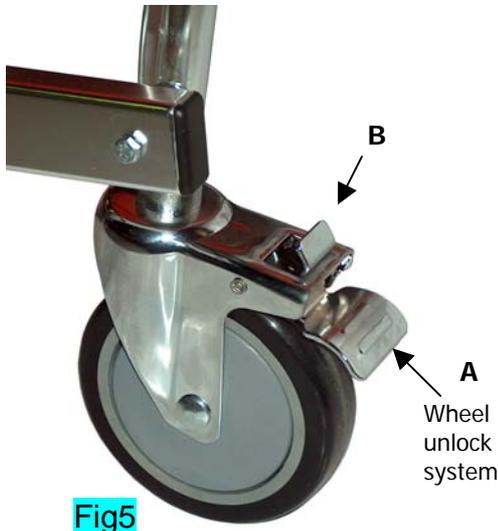

HOW TO FOLD THE WHEEL CHAIR

Bring back all the handles to the initial positions. With one hand pull up the bar as in fig. 7 , with the second hand pull the wheel chair aluminium profile. Pull in as much as possible and the wheel chair will be fully folded as in fig. 1.

For a better security the wheel chair is supplied with a belt which stops any accidental opening

HOW TO KEEP THE WHEEL CHAIR CLEAN AND TO STORE THEM

Using equipment disinfectant solutions. Medical devices . Store them in a clean and dry room far away from direct heat.

Sizes:

Folded : mm.910H x 195P x 520L
Open : mm.910H x 710P x 520L
Weight : 8,50 Kg.
Max load: 150 Kg.